
Alexis™ ViU™

Wound Protector-Retractor



Light off

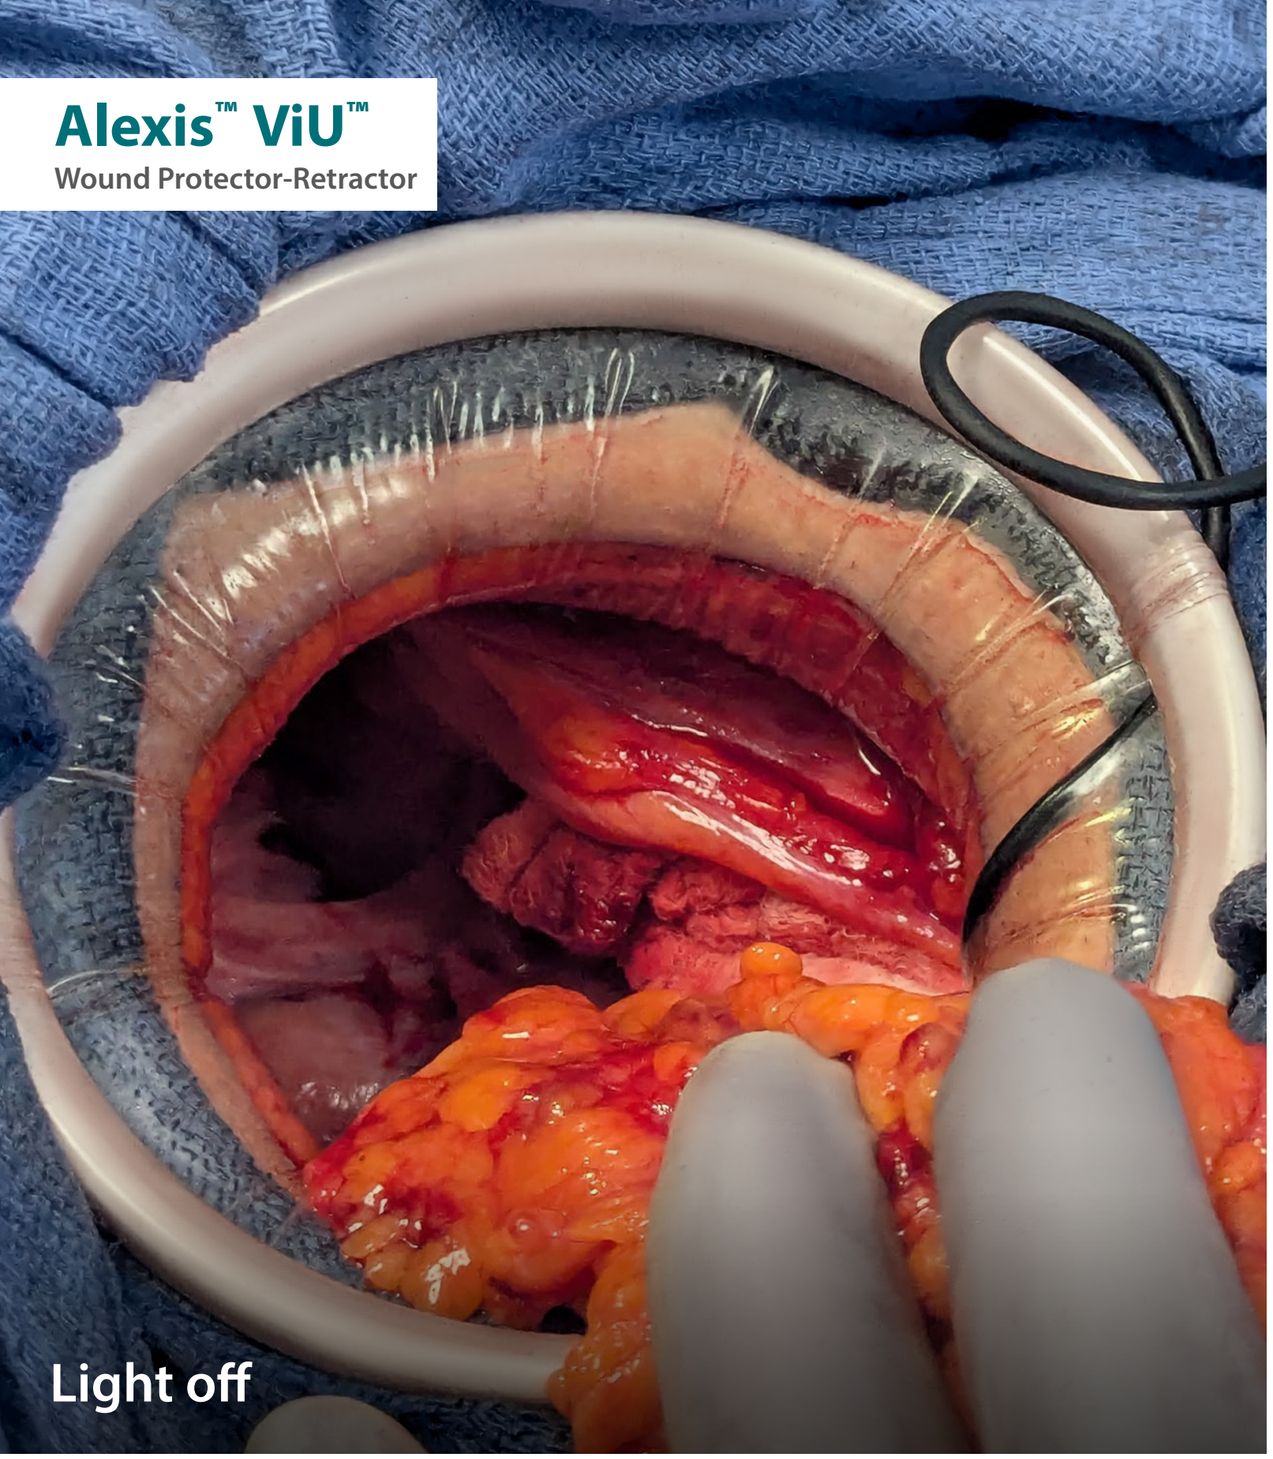

Light on

Erik Noren,
MD, MS, FACS, FASCRS
Sigmoid Resection

Erik Noren is a paid consultant of Applied Medical.

Devices must be administered by a healthcare professional and may not be approved in all markets. Refer to the instructions for use (IFU) for indications, contraindications, warnings, precautions,instructions, and other information.

© 2026 Applied Medical Resources Corporation, Rancho Santa Margarita, California.
Applied Medical, the Applied Medical logo design, and marks designated with the symbol ™ are trademarks of Applied Medical Resources Corporation, registered in one or more of the following countries: Australia, Canada, Japan, South Korea, the United States, the United Kingdom, and/or the European Union.

10/2026 757801-EN-C

Applied Medical